Troubleshooting a Pumping Latch Closed alarm

MedSystem III® infusion pump

Pumping Latch Closed alarms can be reduced with the following practices:

- Turn the pump on before inserting the cassette into the pump
- With tubing down, be sure to use a 45-degree upward motion to insert cassette into channel
- Stop the channel before removing the cassette from the pump
- Fully extend the cassette slide clamp when removing the cassette from the pump *(Figure A)*

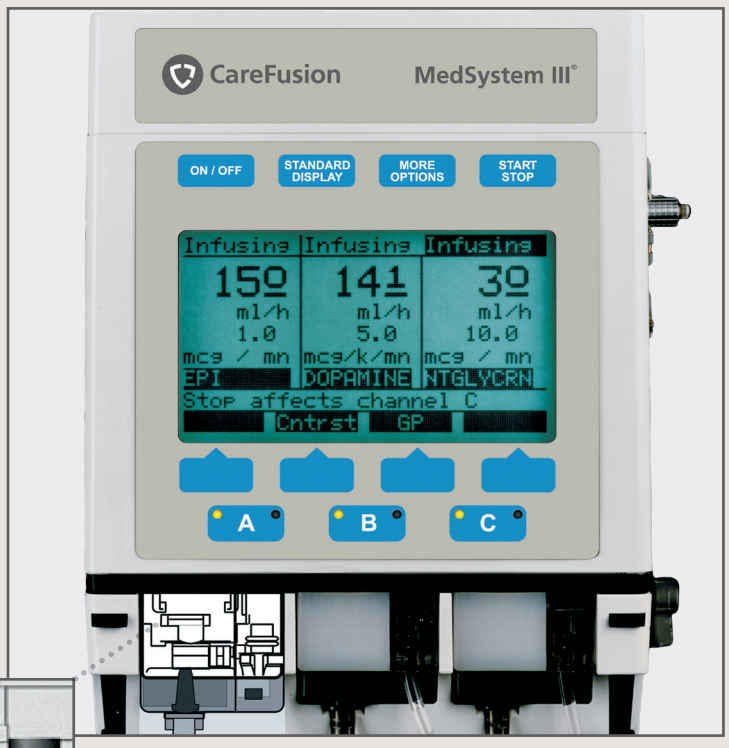

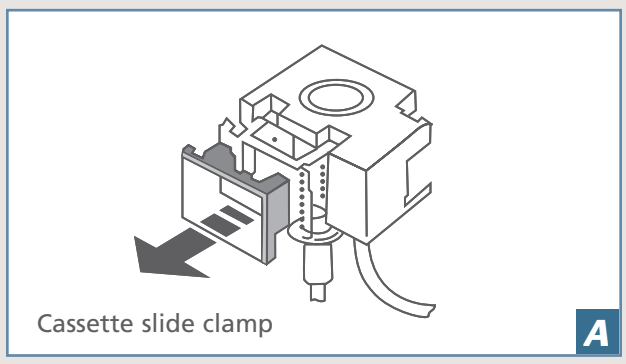

To address a Pumping Latch Closed alarm *(Figure 1):*

- Use only your finger to push down the closed pumping latch jaw until it snaps open *(Figure 2)*
- If the pumping latch jaw is visibly broken, the channel may be disabled by pressing the **Service** key
- **Do not press the Service key unless you wish to disable the channel**

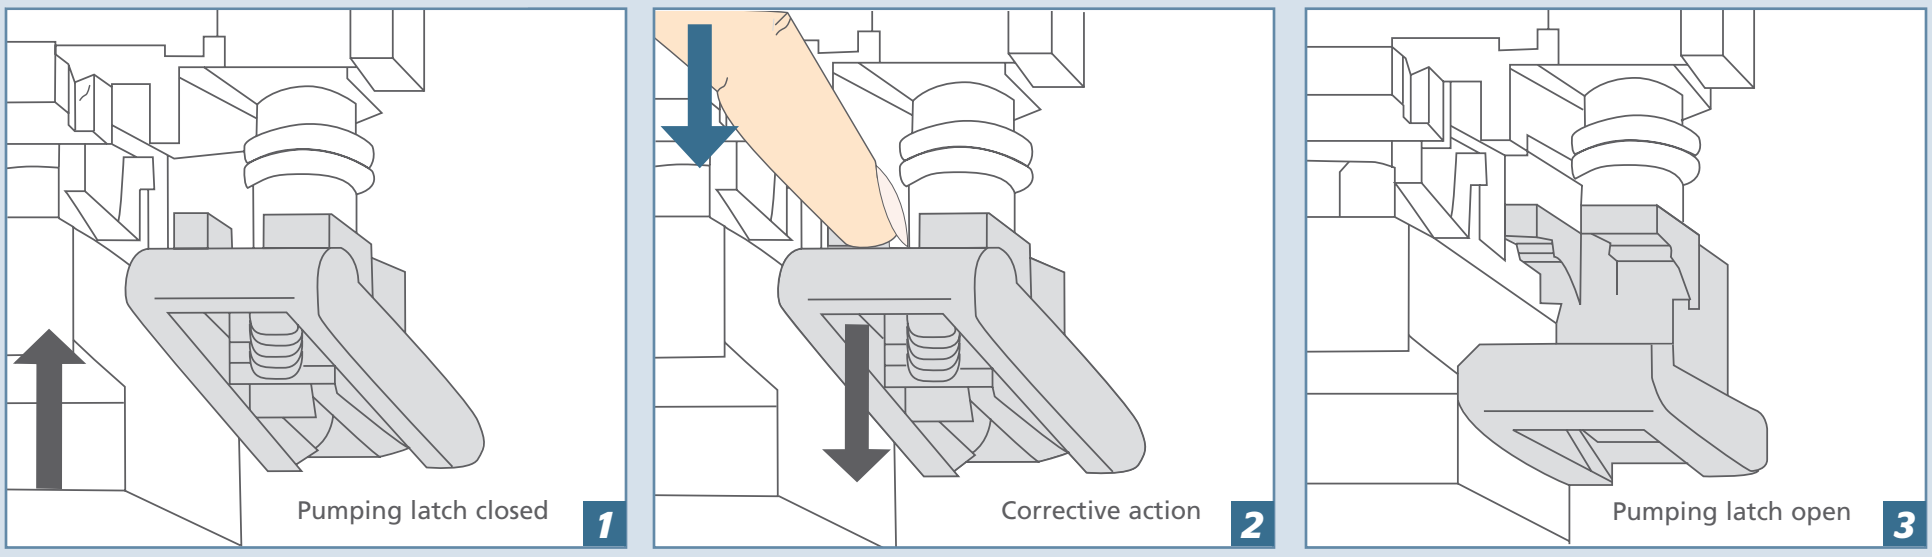

Note: *Illustrations are shown with protective base cover removed.*

For product support, please contact Customer Advocacy at **888.812.3266** or email **customerfeedback@carefusion.com.**
For technical support, please contact Instrument Technical Support at **888.812.3229.**
For product orders, please contact Customer Order Management at **800.482.4822.**

CareFusion
San Diego, CA

carefusion.com

CareFusion

© 2011 CareFusion Corporation or one of its subsidiaries. All rights reserved. Alaris and MedSystem III are trademarks or registered trademarks of CareFusion Corporation or one of its subsidiaries. IF2296-01 (0511/PDF)